

# Biomechanical Comparison of Repair Strength of CoNextions® TR Tendon Repair System and Suture in Digital Flexor Tendons

CoNextions Research & Development

## Objective

The purpose of this study was to compare the tensile strengths of repairs made to transected cadaveric digital flexor tendons with the CoNextions TR Tendon Repair System or a conventional suture repair technique.

## Background

Suture has remained the standard of care for the repair of lacerated or severed tendons since it was first documented over 1800 years ago (Manske 2005). Despite advancements in biomaterials, operative techniques, and rehabilitation protocols, postoperative complications following tendon repair are still common. These complications include rupture of the tendon repair and adhesion formation at the repair site and can lead to long-term restriction of the joint mobility, additional surgical procedures, and extensive rehabilitation (Dy 2012). The CoNextions TR Tendon Repair System was designed to provide an alternative to suture for the repair of tendons. The implant consists of two identical stainless steel anchors implanted simultaneously into the injured tendon. The tendon repair site is centered between the anchors which are connected by two loops of ultra-high molecular weight polyethylene (UHMWPE) fiber (Figure 1).

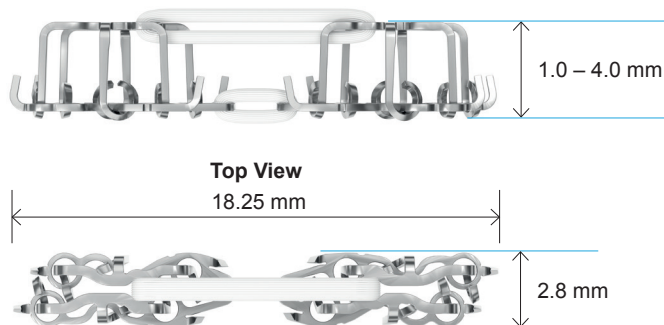


Figure 1: Deployed CoNextions TR Implant

The CoNextions TR implant is provided in two pieces pre-loaded into an Implant Mechanism. During implant deployment the top and bottom pieces of the implant form together securing the reapproximated ends of the injured tendon. The system was designed for the repair of tendons that are less than 4 mm in thickness. The system requires at least 20 mm (10 mm/side) of surgical site access for proper implant deployment.

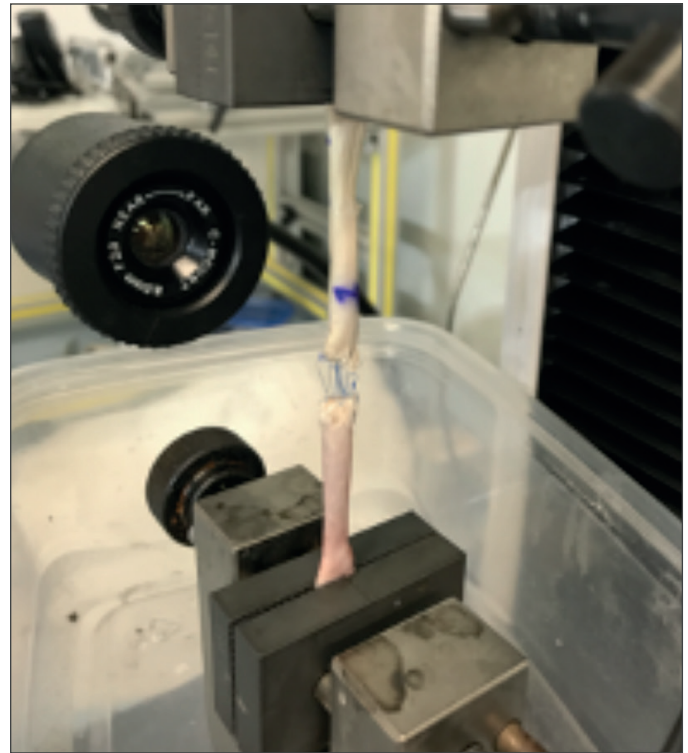


Figure 2: Tensile Test Set-up

## Sample Preparation

Ten (10) flexor digitorum profundus (FDP) tendons at the digit level (Zone 2) and 10 flexor digitorum superficialis (FDS) tendons at the wrist level (Zone 5) from cadaveric specimens were measured and transected at two locations within the specified Zone. One transection was repaired using the CoNextions TR System with the other transection repaired using an 8-strand locked cruciate suture repair using 4-0 FiberLoop® Suture (AR-7249-20, Arthrex, Inc.). All repairs were performed by a fellowship-trained orthopedic hand surgeon.

## Tensile Testing

Samples were excised from the cadaver following the repair procedures and pulled to failure at a rate of 20 mm/min on an Instron® tensile testing machine. (Instron 3342 Series Universal Testing Device, Instron Corporation). The load at 2 mm of displacement (2 mm Gap Force) and ultimate tensile strength were recorded for each sample (Figure 2).

## Results

The failure mode for all test samples was pull-through at the device/soft tissue interface with the exception of one suture FDP repair that had a knot untie. CoNextions TR specimens produced higher 2 mm Gap Forces and Ultimate Tensile Strengths in Zone 2 FDP tendons and Zone 5 FDS tendons (Table 1, Figure 3).

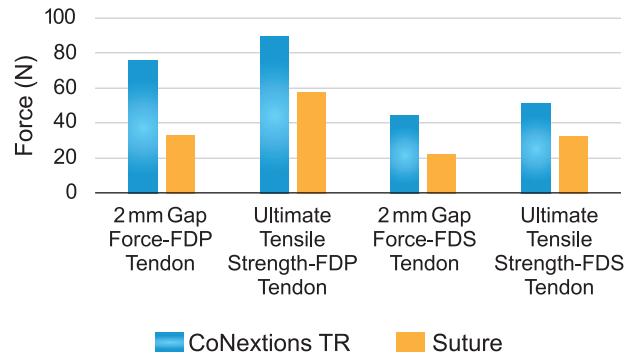


Figure 3: Tensile Testing Results

	FDP Tendons (Zone 2)		FDS Tendons (Zone 5)	
	2 mm Gap Force (N) Mean (STD)	Ultimate Tensile Force (N) Mean (STD)	2 mm Gap Force (N) Mean (STD)	Ultimate Tensile Force (N) Mean (STD)
<b>CoNextions TR</b> (n=9 for both tendons*)	75.3 (19.4)	89.2 (21.0)	44.1 (3.3)	52.1 (6.6)
<b>FiberLoop Suture</b> (n=10 for both tendons)	33.0 (13.5)	57.6 (17.3)	23.2 (3.5)	33.5 (10.8)

Table 1: Summary of Pull Test Results

\*One FDP tendon in the CoNextions TR group was damaged during excision and excluded. Tendon dimensions were not recorded for one FDS tendon in the CoNextions TR group with the results excluded.

Tukey's Pairwise Comparisons concluded Ultimate Force values for CoNextions TR were significantly greater than those for suture for both sets of tendons ( $\alpha=0.05$ ).

## Conclusion

Repairs produced using the CoNextions TR System were significantly stronger than a conventional suture repair technique for the repair of FDP tendons transected in Zone 2 and FDS tendons transected in Zone 5.

## References

Dy CJ, et al. Complications after flexor tendon repair: a systematic review and meta-analysis. J Hand Surg AM 2012;37A:543-51.  
Griffin M, et al. An overview of the management of flexor tendon injuries. Open Orthopaedics Journal 2012;6:28-35.

This document is intended solely for the use of healthcare professionals. Benchtop testing may not be indicative of clinical performance. The information presented is intended to demonstrate a CoNextions Inc. product. CoNextions does not practice medicine and recommends that surgeons be trained in the use of any particular product before using it in surgery. A surgeon must always rely on his or her own professional clinical judgment when deciding whether to use a particular product when treating a particular patient. CoNextions does not dispense medical advice and recommends that surgeons be trained in the use of any particular product before using it in surgery. Individual results will vary based on health, weight, activity and other variables. Not all patients are candidates for this product and/or procedure. Products may not be available in all markets because product availability is subject to the regulatory and/or medical practices in individual markets. Please contact your CoNextions representative if you have questions about the availability of CoNextions products in your area. For indications, contraindications, warnings, precautions, potential adverse effects and patient counselling information, see the package insert or contact your local representative. Visit [www.conexionsmed.com](http://www.conexionsmed.com) for additional product information. CoNextions owns, uses, or has applied for the following trademarks: CoNextions, Coronet, Revolutionizing Tendon Repair. Sawbones is a trademark of Pacific Laboratories Inc. FiberWire is a trademark of Arthrex, Inc. Instron is a trademark of Illinois Tool Works Inc.

**Manufactured by:**  
CoNextions Inc.  
150 North Wright Brothers Drive,  
Suite 560  
Salt Lake City, Utah 84116, USA

Ordering Information/  
Technical Information:  
+1 (385) 351 1461  
[www.conexionsmed.com](http://www.conexionsmed.com)